

Thoracic Electric Bio-Impedance Artifacts Removal by Block Related Adaptive Eliminators for Remote Health Care



Soniya Nuthalapati, Kusuma Nutalapati, Venkata Varun Sai Nallapaneni, Siddabattuni Harinadh, Prem Chand Tallapaneni, T.R Sai Suraj

Abstract: Study of thoracic-electrical- bio-impedance (TEB) simplifies heart attack volume during abrupt cardiac detention. Here in this paper we presented various effective and arithmetically reduced flexible techniques to show high quality TEB element. In scientific circumstances, TEB wave accounts several natural and un-natural events that veil the small things which are needed in finding the depth of the heart attack. In addition to that arithmetical convolution is the significant factor in a present-day wearable health based detecting device. Thus we used a novel signal processing method for TEB improvement in distant health-care structures. To do this we selected higher-order adaptive-filter as an essential component in designing TEB. To boost purifying capacity, merging velocity, to decrease mathematical difficulty of signal processing method, we used information normalization and cutting the data-regressor. The designed applications were checked on original TEB signals and the executed outcome established that the designed regressor eliminated the normalized high order purifier which is apt for a pragmatic health-care structure.

Keywords: Thoracic Electrical Bioimpedance (TEB), adaptive-filter, data regressor, various techniques.

I. INTRODUCTION

The scaled fourier linear combiner [SFLC] process linked with R-R interim of ECG is developed which allows cardio graphic waves and also a mean-squared error [MSE] action for fourier-linear-combiner [FLC] filter is designed easily. Also a time-varying series for least mean square [LMS] method is used to give quick merging and to eliminate the unrelated noise waves during rest, exercise conditions. The technique to calculate motor-unit-number-index [MUNIX], compound muscle action potential [CMAP] and electromyographic [EMG] intrusion design were adopted and found that MUNIX records were low in fragile muscles, also the assessment device depending on 2 system-on-chips (SOC) results for detecting cordial biopotential, electrical bio impedance [EBI] calculation and raspberry PI.

Manuscript received on February 02, 2021.

Revised Manuscript received on February 08, 2021.

Manuscript published on February 28, 2021.

* Correspondence Author

Soniya Nuthalapati*, Department of Electronics and Communication Engineering, JNTUK, Guntur (A.P), India. Email: nuthalapatisoniya@gmail.com

Kusuma Nutalapati, Department of Electronics and Communication Engineering, JNTUK, Guntur (A.P), India. Email: nutalapatikusuma1996@gmail.com

Venkata Varun Sai Nallapaneni, Department of Electronics and Communication Engineering, JNTUK, Guntur (A.P), India.

Siddabattuni Harinadh, Department of Electronics and Communication Engineering, JNTUK, Guntur (A.P), India.

Prem Chand Tallapaneni, Department of Electronics and Communication Engineering, JNTUK, Guntur (A.P), India.

© The Authors. Published by Blue Eyes Intelligence Engineering and Sciences Publication (BEIESP). This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>)

Outcome provided how raspberry PI is used for fast prototyping with almost extensively found and low cost devices. Some more techniques like the utilization of 2-dimensional [2-D] D-bar technology for EI tomography is demonstrated and empirical info is taken on various electrodes of a body and correlated with rebuilds by NOSER method on the same info, an automatic wave refining method, altogether balancing, brought noiseless impedance info that allowed study in rest and exercise condition for general young male person and found that altogether balancing can markedly improve the voltage appropriateness of ICG. In addition the instead of empirical method, numerical approach is done in a 3-dimensional volume and then utilized to find the impact of parallel-tissue-resistance [PTR], catheter location and shrinkage of ventricle, concluded that PTR is having total effect on volume calculations, stroke volume does not change by any of the three aspects. Moreover various capable and easy adaptive techniques were proposed to show high-quality thoracic-electrical-bioimpedance [TEB] factor. To enhance purification of signals the data normalization is applied and data regressor is clipped and found that it is applicable for pragmatic healthcare structure. To reduce the difficulty, the techniques like the use of electrical-impedance-tomography [EIT] the current is implanted in to a person with different electrodes and sketched the image of inner resistivity circulation and found that it is most suited for motion-noise as compared to sleep tracking process and the to analyze cordial waves a time-frequency evaluation technique is provided and concluded that it gave exact results than previous ones in decreasing ventilation and motion noise, a mathematical approach is used in making a digital IIR band-pass-filter and tested on 4 male persons during exercise and come forth that it is usable to track cordial activity during workout. For the calculation optimization, the impedance calculation is done with subject thorax from 9.6 KHz to 614 KHz and its variation for cordial, panting periods were noted and concluded that impedance dropped to 64.0% of low frequency and also by utilizing bisyncytial design of heart, time elements of QRS, QRS-T were linked with amplitude (A), area (μ), activation time (τ) of action potential (AP) around the ventricles. μ and τ are the outcomes to inverse problem for general heart. With the enhancement of philosophical model of conductivity of pulsatile gore passing over rigid tubes is studied during cardiac period and came up that conductivity corresponds with spatial equate gore tempo along with fidelity.



Thoracic Electric Bio-Impedance Artifacts Removal by Block Related Adaptive Eliminators for Remote Health Care

A linear electrode array is used to calculate electrical impedance [EI] during the variations of blood quantity in trunk and resulted that the EI signal may be detached in time, position on trunk and aortic sound variations were detected exactly.

to calculate 2-D impedance magneto cardiograms [I-MCGs] and MCGs over the heart in concert is proposed and the waves are noted using superconducting-interference-device (SQUID) method and concluded that the basic 2-D I-MCG wave can give more logical info on rotating action of heart. During laying down, sitting and workout conditions, the band and local electrode waves were calculated and found that the local electrodes may not provide same stroke sound info though they are essential in calculating local movements of pivotal flow. In this the noise can be generated using the finite element model [FEM] is employed to compute the result of chest elaboration on recreated conductivity figures. Due to trunk enlargement a noise is formed which made the lungs to come nearer. With finite contrast approach, the grant of different causes to impedance-cardiogram [ICG] were noted for primitive band electrode structure and suggested that the trunk ICG wave is blended depiction of various integral aspects and cannot be steady for stroke sound estimation. during stress state, to record cordial output the ICG is improved and testing is done using spot electrode [SE] and concluded that SE array was 13.6 to 45.5% vast than the band electrode [BE] in rest and 4 stages of workout and hence can be put in the place of BE. To track cardiopulmonary-resuscitation [CPR] defibrillators were invented to place outside, trunk impedance variations are almost related to lung sound changes and can track the ventilator action, exact ventilation analysis during CPR is achieved. The new techniques like Zink, a standalone-bio impedance analyst using IoT tracking features is defined, monitored in real-time and concluded that it is apt for medical, personal health IoT tracking appliances. A combination of seismo cardiogram (SCG) and gyro cardiogram (GCG) is studied using MEMS and proved that instead of taking only GCG wave it is better to take first derivative of GCG with SCG. An enhanced ICG is used to record the cordial waves during workout on 10 subjects and compared with resting condition, as correlation-co-efficient among BEICG and rest is 0.96 and among SEICG and rest is 0.90 which can be upgraded to 0.95 by using peak-to-valley length in place of peak length.

II. IMPROVEMENT OF THORACIC ELECTRO BIO-IMPEDANCE (TEB) SIGNALS THROUGH ADAPTIVE TECHNIQUES:

In the practical health care situations the signals gets polluted with the noise such that we have to separate the signal and noise and to take out the actual signal back. The artifacts that involved are Respiratory Noise (RN) and Muscle noise (MN). Here the conceptual constraints are non-stationary, so with the help of adaptive filters we can extract the purified signal. In this the feed in is TEB signal taken from respective electrodes. The known system here is a six lead such that we have to note down the signal at 250Hz through a 12bit analog to digital converter (ADC), leads to normalization such that we can recognition the type of artifact it is. Here we can calculate the power spectral density (PSD) and correlated that value with mentioned signal of that artifact and connects to the Signal Improvement Block (SIB). For this reason, we have to take

the mentioned alternator which has different number of signals with artifacts. Later on artifact recognition this is given to the SIB. The corresponded polluted parameter is injects as mentioned to SIB. The block diagram of SIB is shown in Fig.1. The SIB contains FIR (Finite Impulse Response) filter and the weight modernized structure to modernize weight concertions.

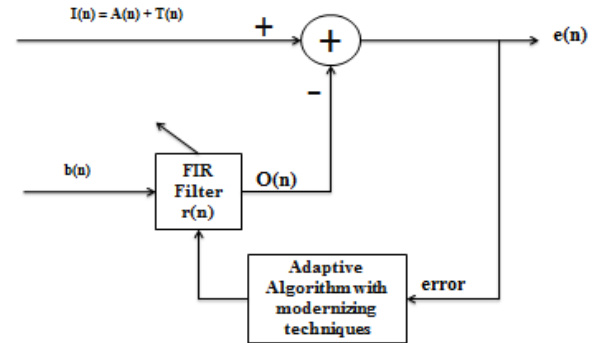


Figure 1:Representation of Signal Improvement Block (SIB)

So a LMS-related adaptive filter with the filter length named as L. The feed in signal to SIB is taken as I(n). Since this is thoracic electric bio impedance signal such that we have to take the impedance collective as A(n) and artifact elemental as T(n). Hence b(n) is the correlated mentioned signal considered from mentioned generator say r(n) is the impulse output of FIR filter, O(n) is the resultant of FIR filter, e(n) is the error occurred in the SIB. The weight modernize appliance of LMS algorithm

$$r(n+1) = r(n) + 2 Z I(n) e(n) \quad (1)$$

at which $r(n) = [r_0(n), r_1(n), r_2(n), \dots, r_L(n)]^T$ is the egress weight vector components at the n^{th} value, and $I(n) = [I(n), I(n-1), \dots, I(n-L+1)]^T$ is the feed in progression, and $e(n) = I(n) - r(n)b(n)$ is the Least Mean Square (LMS) technique and 'Z' is the step size constraint. The optimized adaptive techniques along with data clipping, and leads to reduce the mathematical difficulty. The obtained technique is Data Clipping LMS (DCLMS). Such that the weight modernize equation for this can be represented as

$$r(n+1) = r(n) + 2 Z \text{CLP}\{I(n)\} \{e(n)\} \quad (2)$$

at which the function $\text{CLP}\{\cdot\}$ can be known as clipping that is

$$\text{CLP}\{e(n)\} = \begin{cases} 1 & : e(n) > 0 \\ 0 & : e(n) = 0 \\ -1 & : e(n) < 0 \end{cases} \quad (3)$$

To enhance the convergence rate, filtering ability and to minimize mathematical difficulty, we have to substitute normalization to LMS and DCLMS techniques as Data Normalized LMS (DNLMS) and Data Clipping Normalized LMS (DCNLMS) techniques. Their weight modernize equations are

$$r(n+1) = r(n) + 2Z(n)I(n)e(n) \quad (4)$$

$$r(n+1) = r(n) + 2Z(n)\text{CLP}\{I(n)\} \{e(n)\} \quad (5)$$

at which $Z(n)$ is the fickle step size relates feed in data repeatedly, and that follows as

$$Z(n) = \frac{Z}{d + I^t(n)I(n)} \quad (6)$$

The constraint 'd' is to optimize the denominator value, and then step size becomes too large.

The DNLMS gives faster response because of variable step size in weight modernized relation. The DNLMS is better than DCNLMS, because of clipping. The multiplication in numerator of DCNLMS is self-reliant of filter length themes as advantage. LMS is better than DCLMS because of optimized multiplications equal to its filter span. Data clipping reduce multiplications, mainly in VLSI design, like chip design in wearable device. We optimized '3' number of multiplications from $L+3$ in LMS. If M is large, DCLMS is useful and DCNLMS totally removes multiplications and more reliable in practical.

Table1 Correlated table for various techniques in terms of mathematical calculations

Technique	Multiplications	Additions	Addition with Sign Check
LMS	$L+3$	$L+1$	Nil
DCNLMS	3	$L+1$	Nil
DCNSRLMS	L	$L+1$	Nil
BBDCNSRLMS	Nil	Nil	$L+3$

In previous studies, the sign related techniques heavily reduce the multiplication and accumulation (MAC) operations, and to eliminate noise from TEB signal. The projected algorithms still have optimized computations so, the block related techniques with step size is applied. We will separate key signal as different portions. And pick the maximum impact portion for the computation of 'Z'. The equations are

$$r(n+1) = r(n) + 2Z(n) \text{CLP}(\{\text{sgn}(I(n))\}\{e(n)\}) \quad (7)$$

Equation (7) is Data Clipping Normalized Sign LMS (DCNSLMS). The signum function applied to key signal

$$r(n+1) = r(n) + 2Z(n) \text{CLP}(\{I(n)\}\{\text{sgn}(e(n))\}) \quad (8)$$

Equation (8) is Data Clipping Normalized Sign Regressor LMS (DCNSRLMS). Here the signum function is applied to error signal.

$$r(n+1) = r(n) + 2 \frac{Z}{d + I^2(n)} \text{CLP}(\{\text{sgn}(I(n))\}\{\text{sgn}(e(n))\}) \quad (9)$$

Equation (9) is Block Based DCNSRLMS (BBDCNSRLMS). Here computations like multiplications, additions and other operations gets optimized and self-reliant on filter span.

III. SIMULATION RESULTS:

The projected techniques are efficient in health care conditions, and checked through TEB and compared with reported MIT-BIH arrhythmia databases. The TEB is stored in kendall ARBO H98SG electrocardiogram electrodes. In this analysis the projected techniques studied the signal to noise ratio improvement (SNRI), Misadjustment (MSD) and Excess Mean Square Error (EMSE) for the ten evaluations, those are normalized and checked with traditional LMS related SIB. These constraints are categorized in Tables 2-4 and analyzed in dBs. To show vacuity effect, as Gaussian blare with divergence 0.001 summed to TEB in biotelemetry structure. The obtained five resultants are I, II, II, IV and V.

These values are polluted with artifacts RN and different SIBs TEB improvement done through LMS, DCLMS, DCNLMS, DCNSLMS, DCNSRLMS and BBDCNSRLMS techniques.

a) Adaptive removal of RN artifacts: The feed in TEB elemental signal with RN is given to SIB as shown in Figure 1. The remark a, pollutant elemental, ties in with artifact instant in key abundance of SIB, removes the error function and improves the concertion of FIR filter. The modernizing filter weights and techniques generates remark signal highly ties in with original polluted elemental and gets revoke. The outcomes are resulted in Figure2-5. The performance of this employment is related with remark to the SNRI, MSD and EMSE are categorized in Tables 2-4. In regard to SNRI the BBDCNSRLMS algorithm is good compared to another technique. These technique goals SNRI of 9.7936 dB. While for EMSE and MSD calculations, BBDCNSRLMS related signal improvement is higher than another employment.

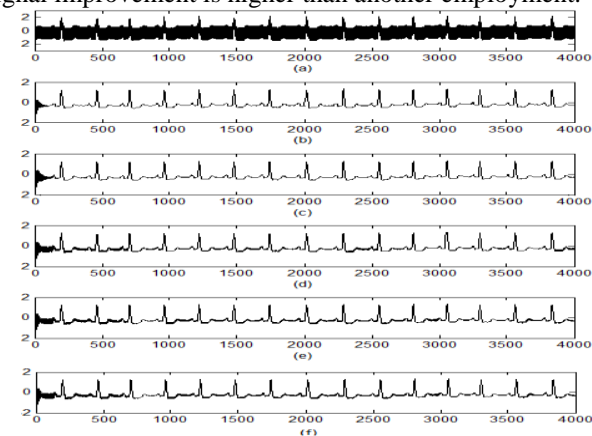


Figure 2: Representation of TEB improved outcome through LMS and its alterations for RN removal a) Actual TEB wave b) TEB wave with RN c) Decontaminated wave through LMS related SIB d) Decontaminated wave through DCNLMS related SIB e) Decontaminated wave through DCNSRLMS related SIB f) Decontaminated wave through BBDCNSRLMS related SIB.

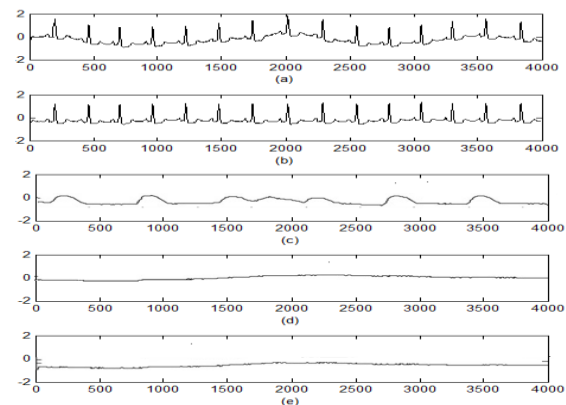


Figure 3: Wave of Revoked RN noise from Residual noise a) Actual RN elemental b) Residual noise succeeding LMS technique c) Residual noise succeeding DCNLMS technique

Thoracic Electric Bio-Impedance Artifacts Removal by Block Related Adaptive Eliminators for Remote Health Care

d) Residual noise succeeding DCNSRLMS technique e) Residual noise succeeding BBDCNSRLMS technique

a) Adaptive Removal of MN Artifact: The TEB signal with MN is feeder as in to the SIB unit as visualized in Fig.1. The artifact occurred due to muscle movement. The simulation outcomes are visualized in Fig.4. The achieved outcomes are computed, normalized for ten times and visualized in Tables 2-4.

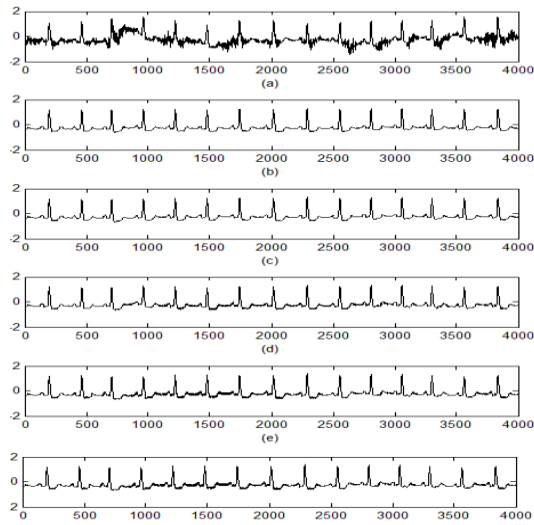


Figure 4: Representation of TEB improved outcome through LMS and its alterations for MN removal a) Actual TEB wave b) TEB wave with MN c) Decontaminated wave through LMS related SIB d) Decontaminated wave through DCNLS related SIB e) Decontaminated wave through DCNSRLMS related SIB f) Decontaminated wave through BBDCNSRLMS related SIB

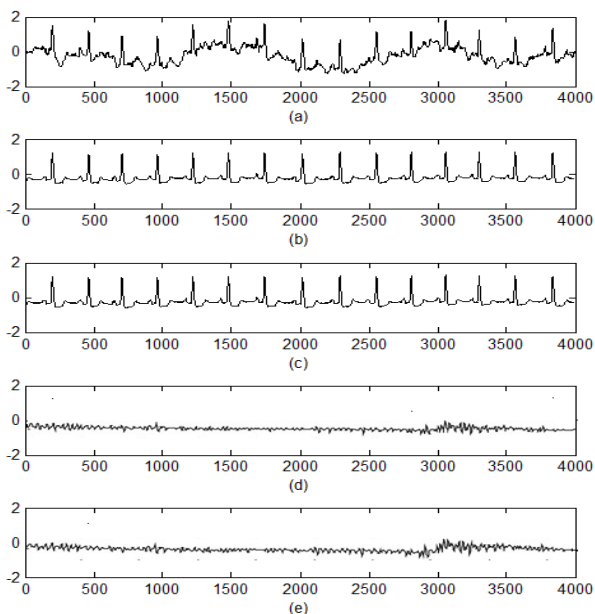


Figure 5: Wave of Revoked MN noise from Residual noise a) Actual MN elemental b) Residual noise succeeding LMS technique c) Residual noise succeeding DCNLS technique d) Residual noise succeeding DCNSRLMS technique e) Residual noise succeeding BBDCNSRLMS technique This visualizes BBDCNSRLMS related noise removal is good over the other techniques. The medium SNRI for DCNSRLMS and BBDCNSRLMS in the improvement procedure is calculated as 9.7936 and 10.3262 dB

correspondingly. Fig.5 visualizes the residual noise elemental subsequence to MN elimination

Table2 Signal to Noise Ratio Improvement (SNRI) values in dBs for different techniques in SIB

Artifact Type	Data Number	LMS	DCNLS	DCNSRLMS	BBDCNSRLMS
RN	101	2.6345	8.9795	9.3946	9.5678
	102	3.4241	9.2781	9.9332	9.7816
	103	3.5525	8.5259	9.7817	9.6541
	104	3.3458	8.7929	9.9873	9.9891
	105	3.3191	8.9914	9.6828	9.9754
	Average	3.2552	8.9135	9.7559	9.7936
MN	101	3.7893	8.6435	9.3499	9.6543
	102	4.9535	9.2913	10.6641	10.9987
	103	4.9653	9.4337	10.6997	10.9965
	104	3.9729	9.1573	9.9429	10.1949
	105	3.6384	9.8775	9.9672	9.7864
	Average	4.2638	9.2806	10.1247	10.3262

Table 3 Misadjustment (MSD) values in dBs for different techniques in SIB

Artifact Type	Data Number	LMS	DCNLS	DCNSRLMS	BBDCNSRLMS
RN	101	0.2678	0.2499	0.2347	0.1998
	102	0.0559	0.0466	0.0316	0.0235
	103	0.0507	0.0410	0.0356	0.0345
	104	0.1406	0.1208	0.1047	0.0987
	105	0.1789	0.1586	0.1176	0.1068
	Average	0.1387	0.1233	0.1048	0.0926
MN	101	0.4751	0.4268	0.3715	0.0213
	102	0.1157	0.1069	0.1019	0.0989
	103	0.0946	0.0839	0.0712	0.0619
	104	0.1307	0.2009	0.1939	0.1843
	105	0.1764	0.1436	0.1126	0.1029
	Average	0.1985	0.1924	0.1702	0.0938

Table 4 Excess Mean Square Error (EMSE) values in dBs for different techniques in SIB

Artifact Type	Data Number	LMS	DCNLS	DCNSRLMS	BBDCNSRLMS
RN	101	-14.6543	-17.5089	-20.8129	-20.9987
	102	-15.0139	-18.3773	-22.2971	-22.3421
	103	-14.8669	-17.9926	-21.9359	-21.9654
	104	-14.1379	-16.9356	-20.2793	-20.3329
	105	-16.1123	-20.9399	-23.2354	-23.3369
	Average	-14.9570	-18.3508	-21.7121	-21.7950
MN	101	-12.7959	-14.2859	-16.5173	-16.6284
	102	-11.9964	-13.6123	-15.7134	-15.8845
	103	-10.9553	-12.8137	-14.5462	-14.6573
	104	-11.8864	-13.9399	-19.2999	-19.3096
	105	-15.3143	-18.5448	-16.2869	-16.3979
	Average	-12.5896	-14.6393	-16.4727	-16.5760

IV. CONCLUSION:

In this work, we have proposed some effective SIBs for distant healthcare auditing systems. To enhance the capability of projected SIBs, we enforced the practical TEB signals for enhancement.



To establish cohesion, convergence rate, filtering and optimized mathematical difficulty, we composited the aspects of maximum order filtering, clipping data regression and block based enhancement.

So from the outcomes it is clearly stated BBDCNSRLMS gives the best outcomes over the other techniques. The main improvements of this technique are speedy convergence, good filtering ability due to fickle stepsize and optimized mathematical calculations due to clipping and block division. So it is concluded that this technique gives good results and opted for distant health care auditing usances.

REFERENCES:

1. Allan Kardec Barros, "Filtering Noncorrelated Noise In Impedance Cardiography", IEEE Transactions on Biomedical Engineering, Vol. 42, No. 3, March 1995, pp. 324-327.
2. Allan Kardec Barros, "MSE Behavior of Biomedical Event-Related Filters", IEEE Transactions on Biomedical Engineering, Vol. 44, No. 9, Sep. 1997, pp. 848-855.
3. Roger Dzwonczyk, "Myocardial Electrical Impedance Responds To Ischemia and Reperfusion in Humans", IEEE Transactions on Biomedical Engineering, Vol. 51, No. 12, Dec. 2004, pp. 2206-2209.
4. Abdelakram Hafid, "Full Impedance Cardiography measurement device using Raspberry PI3 and System-on-Chip biomedical Instrumentation Solutions", IEEE Journal of Biomedical and Health Informatics, Vol. 22, Iss. 6, Nov. 2018, pp. 1883 – 1894.
5. David Isaacson, "Reconstructions of Chest Phantoms by the D-Bar Method for Electrical Impedance Tomography", IEEE Transactions on Medical Imaging, Vol. 23, No. 7, July 2004, pp. 821-828.
6. Michael Muzi, "Computer-Automated Impedance-Derived Cardiac Indexes", IEEE Transactions on Biomedical Engineering, Vol. 33, No. 1, Jan. 1986, pp. 42-47.
7. Rodney W. Salo, "Measurement of Ventricular Volume by Intracardiac Impedance: Theoretical and Empirical Approaches", IEEE Transactions on Biomedical Engineering, Vol. 33, No. 2, Feb. 1986, pp. 189-195.
8. Muhammad Zia Ur Rahman, "Processing techniques for human thoracic electrical bio-impedance signal in remote healthcare systems", Healthcare Technology Letters, Vol. 3, Iss. 2, June 2016, pp. 124 – 128.
9. Eung Je Woo, "Measuring Lung Resistivity Using Electrical Impedance Tomography", IEEE Transactions on Biomedical Engineering, Vol. 39, Iss. 7, July 1992, pp. 756 – 760.
10. Xiang Wang, "An Advanced Signal Processing Technique For Impedance Cardiography", IEEE Transactions on Biomedical Engineering, Vol. 42, No. 2, Feb. 1995, pp. 224-230.
11. Y. Yamamoto, "Design and Implementation of a Digital Filter For Beat-by-Beat Impedance Cardiography", IEEE Transactions on Biomedical Engineering, Vol. 35, No. 12, Dec. 1988, pp. 1086-1090.
12. Brian Hilton Brown, "Cardiac and Respiratory Related Electrical Impedance Changes in the Human Thorax", IEEE Transactions on Biomedical Engineering, Vol. 41, No. 8, August 1994, pp. 729-734.
13. L. Djordjevic, "Use of Time Integrals of the ECG to Solve the Inverse Problem", IEEE Transactions on Biomedical Engineering, Vol. 32, No. 1, January 1985, pp. 69-73.
14. R. L. Gaw, "The Electrical Impedance of Pulsatile Blood Flowing through Rigid Tubes: A Theoretical Investigation", IEEE Transactions on Biomedical Engineering, Vol. 55, No. 2, February 2008, pp. 721-727.
15. E. Hoetink, "Imaging of Thoracic Blood Volume Changes During the Heart Cycle With Electrical Impedance Using a Linear Spot-Electrode Array", IEEE Transactions on Medical Imaging, Vol. 21, No. 6, June 2002, pp. 653-661.
16. Akihiko Kandori, "Two-Dimensional Mapping of Impedance Magnetocardiograms", IEEE Transactions on Biomedical Engineering, Vol. 49, No. 7, July 2002, pp. 721-728.
17. Robert P. Patterson, "Impedance Cardiography Using Band and Regional Electrodes in Supine, Sitting, And During Exercise", IEEE Transactions on Biomedical Engineering, Vol. 38, No. 5, May 1991, pp. 393-400.
18. Andy Adler, "Impedance Imaging of Lung Ventilation: Do We Need to Account for Chest Expansion?", IEEE Transactions on Biomedical Engineering, Vol. 43, No. 4, April 1996, pp. 414-420.
19. Li Wang, "Multiple Sources of the Impedance Cardiogram Based on 3-D Finite Difference Human Thorax Models", IEEE Transactions on Biomedical Engineering, Vol. 42, No. 2, Feb. 1995, pp. 141-148.
20. Minghai Qu, "Motion Artifact From Spot And Band Electrodes during Impedance Cardiography", IEEE Transactions on Biomedical Engineering, Vol. 33, No. 11, Nov. 1986, pp. 1029-1036.
21. Martin Risdal, "Impedance-Based Ventilation Detection during Cardiopulmonary Resuscitation", IEEE Transactions on Biomedical Engineering, Vol. 54, No. 12, Dec. 2007, pp. 2237-2245.
22. Luis M. Vela, "Standalone IoT Bioimpedance device supporting real-time online data access", IEEE Internet of Things Journal, Vol. 6, Iss. 6, Dec. 2019, pp. 9545 – 9554.
23. Chenxi Yang, "Combined Seismo- and Gyro-cardiography: A More Comprehensive Evaluation of Heart-Induced Chest Vibrations", IEEE Journal of Biomedical and Health Informatics, Vol. 22, Iss. 5, Sept. 2018, pp. 1466 – 1475.
24. Yujian Zhang, "Cardiac Output Monitoring by Impedance Cardiography during Treadmill Exercise", IEEE Transactions on Biomedical Engineering, Vol. 33, No. 11, Nov. 1986, pp. 1037-1042.

AUTHORS PROFILE



N. Soniya, Assistant Professor received her B.Tech degree from KKR & KSR Institute of Technology and Sciences, Vinjanampadu, Guntur (Dt), Andhra Pradesh and M.tech from KKR & KSR Institute of Technology and Sciences, Vinjanampadu, Guntur (Dt), Andhra Pradesh. And have 3 years of teaching experience as an Assistant professor in various engineering colleges. Currently working as an

Assistant professor in Department of ECE in KKR & KSR Institute of Technology and Sciences, Vinjanampadu, Guntur (Dt), Andhra Pradesh, India. Totally 11 publications are there in various journals. Areas of interests are VLSI, Signal Processing, and wireless communication.



N. Kusuma, Assistant Professor received her B.Tech degree from Vasireddy Venkatadri Institute of Technology and Sciences, Nambur, Guntur (Dt), Andhra Pradesh. And have 3 years of teaching experience as an Assistant professor in various engineering colleges. Currently working as an Assistant professor in Department of ECE in Hindu College of Engineering and Technology Amaravathi

Road, Guntur (Dt), Andhra Pradesh, India. Totally 04 publications are there in various journals. Areas of interests are VLSI, Signal Processing, and wireless communication.