


Measurement of Bone Density Parameters using Ultrasound and Hardware Development on bone Density Measurement

Kunal Khosla, Apurva Naik



Abstract: Ultrasound waves due to their inherent small wavelength can be used in diagnosis or evaluation of tissue. Ultrasound simulations can be useful to investigate and analyze different properties at different sites especially when there is no volumetric data available. In the proposed paper, simulation of ultrasound in a 2-D bone model and hardware implementation has been presented. Due to complex structures of bone, a simple linear model consisting of both cortical and cancellous bone has been proposed. In the simulation, a broadband emitter with center frequency of 1 Megahertz is used along with an array of receivers to capture the signal. An attempt has been made to calculate bone density parameters in-vivo for human feet, and finally display the computed parameters onto a LCD using Arduino Uno Board. An algorithm involving fourier transforms was used to calculate Broadband Ultrasound Attenuation (BUA) and Speed of Sound (SoS) in Matrix Laboratory (MATLAB).

Keywords: Broadband ultrasound attenuation, speed of sound, simsonic, matrix laboratory, osteoporosis, osteopenia, quantitative ultrasound.

I. INTRODUCTION

Use of ultrasound frequencies has the diagnostic capabilities of tissue monitoring, because it can penetrate the bulk, due to its small wavelength. Its diagnostic capabilities include Non- Destructive testing (NDT), tissue healing and foetal health monitoring. There are many commercial devices available in the market which can be used to measure T-Score and Z- Score, like the Mini Omni Portable bone density device by Beamed which applies the probe onto the tibia and wrist and the Sonost-2000 by osteosys which is heel densitometer. Dual Energy X-Ray Absorptiometry (DEXA) scan which is considered a gold standard in bone density measurement, measures bone density at various sites, including the hip, vertebrae etc. Quantitative Computed tomography (QCT) utilizes X-rays at various angles to take measurements and produce images which are finally stitched together to give you a final image. It is used in assessment of risk of fractures.

Biot's theory derives the equations of wave propagation in porous media. The idea of Biot's theory was that the outcome of an incident sound wave onto a porous solid was a fast, slow wave along with a shear wave [3], [4]. Some success has been achieved in modelling sound waves in cancellous

bone using different forms of biot's theory. Except frequencies greater than 1 MHz, biot's theory should be applicable as the wavelengths of the order of 1.5 mm at 1 MHz are larger than the pore size in bones [5, p. 3286].

A. Bone Models and their material constants

The densities [1, p. 195] and elastic constants [1, p. 195] can be used as inputs for building nominal bone models [1, p. 195]. The constants for cortical bone used here were homogenized (average properties of hard tissue and pores [1,p. 194]) and transversely anisotropic. The values of density and elastic constants C_{11} , C_{22} , C_{12} and C_{66} for cortical has been taken from [1, p. 195]. Osteoporotic bones were simulated by reducing the thickness of the cortical bone and changing the densities and elastic constants of the trabecular bone [1,p. 218]. The cortical bone was considered to be perfectly linear in shape, disregarding any curvature which can be responsible for change in BUA values. For cancellous bone, the data has been taken from [2, p. 667]. 1.6 g/cm³ and 1.85 g/cm³, are assumed to be densities of an osteoporotic and normal subject respectively. Elastic constants C_{22} , C_{66} and C_{12} were derived from C_{11} and C_{44} using Lamé parameters μ , λ and equations 1 and 2. The data for density is inconsistent as cortical and cancellous bone density cannot be same because cortical bone is more dense, however the density for osteoporotic subjects is lower than normal, which has been included in these models and one can observe the changes in attenuation values.

$$C_{11} = C_{22} = \lambda + 2\mu \quad (1)$$

$$C_{44} = \mu \quad (2)$$

For example, the 2-D plate bone model for an osteoporotic subject has been shown in "Fig. 1".

B. Simulation Components

To study the nature of bone, a 2-D plate model with cortical and cancellous bone both were drawn. This model can be used to assess the mechanical properties for osteoporotic or normal conditions at different bone sites. In this Simulation,

Manuscript published on 30 August 2019.

*Correspondence Author(s)

Kunal Khosla, Department of Technology, from MIT World Peace University,

Dr. Apurva Naik, Department of Technology Electronics from Shivaji University, Kolhapur

© The Authors. Published by Blue Eyes Intelligence Engineering and Sciences Publication (BEIESP). This is an open access article under the CC-BY-NC-ND license <http://creativecommons.org/licenses/by-nc-nd/4.0/>

Measurement of Bone Density Parameters using Ultrasound and Hardware Development on bone Density Measurement

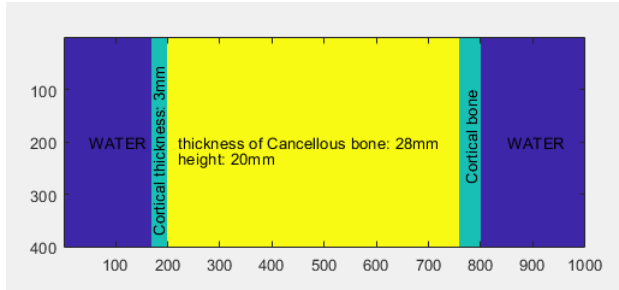


Fig. 1. 2-D Bone plate model

simsonic uses elastic constants and densities as parameters for laying the foundation of nominal bone model. To study the bone density parameters, of cortical and cancellous bones, a 2-D plate model with the dimensions of the calcaneus, if not there exact anatomy had been drawn. In the workstation, separate directories have been assigned for simulation for sample and reference signals. A broadband emitter with centre frequency of 1 MHz is used along with an array of receivers to capture the signal. The calculation of broadband ultrasound attenuation uses the slope of attenuation versus frequency in the range 200 KHz to 600 KHz. BUA is a measure of frequency dependence of the attenuation of ultrasound measured in decibels/megahertz (dB/MHz) and SoS is the speed of ultrasound in the sample expressed in meters/second (m/s). Attenuation, velocity can be found out by computing the fourier transform as per formulas in [6, p. 158,159] which are 3, 4, 5 and 6. Equation 3 was multiplied by 20 to convert the value into decibels.

$$(3) \quad BUA(f) = \frac{A_r(f)}{A(f)}$$

$$(4) \quad \Phi(f) = \arctan \frac{A(f)}{A_r(f)}$$

$$(5) \quad v(f) = \frac{1}{\frac{1}{v_0} \frac{\Phi(f)}{2\pi f l}}$$

$$(6) \quad UBV(f_c) = v(f)$$

where A_r is the amplitude spectrum of specimen in water, A is amplitude spectrum with water alone. $V(f)$ is the phase velocity, v_0 is velocity of sound in water, f/f_c is the frequency/centre frequency, UBV is the ultrasound bone velocity and l is the length of the specimen. Stiffness index can be calculated with the help of 7 used in the Achilles system.

$$(7) \quad SI = 0.67 * BUA + 0.28 * SOS - 420$$

where SoS , BUA are the speed of sound and broadband ultrasound attenuation respectively. The plot of frequency

dependent attenuation was obtained as in “Fig. 2” for a normal subject and in figure “Fig. 3” for osteoporotic subject. The slope of the linear portion (BUA) was obtained in the range 500 KHz to 700 KHz .

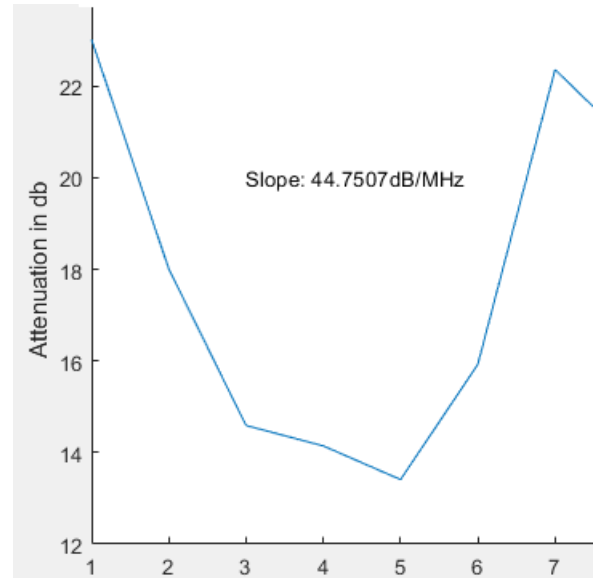


Fig. 2. Broadband Ultrasound Attenuation in a normal bone sample

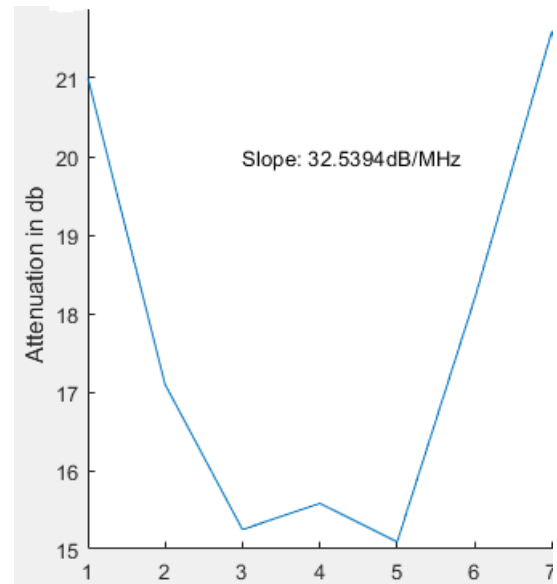


Fig. 3. Broadband Ultrasound Attenuation in an osteoporotic bone sample

C. Methods

The method used here is through mode of transmission and other methods like guided waves or axial transmission can also be used to assess bone condition. In the latter approach the emitter and receiver are on the same side of the specimen.



Bone acts as a waveguide in this mode where the wave travels across the surface to finally reach the receiver.

The tibia, wrist (arm) etc. are popular sites for measurement of bone density using axial transmission while the calcaneus is considered an ideal position for measurement using a pulse through technique. The length of the cortical part in the model of calcaneus was taken to be 1.5 mm close to the value of 1.4 mm in [7]. The length for cancellous part in normal subjects was considered to be 30 mm and 28 mm for osteoporotic subjects. Velocity was calculated with the help of 5 and 6.

II. HARDWARE DEVELOPMENT

The hardware setup in “Fig. 4” has a MHF-400 pulser receiver by Roop Telsonic,



Fig. 4. Hardware setup for Non-Destructive Evaluation in through transmission mode, Courtesy: Cummins College of Engineering Pune

Tektronix TBS 1062 Digital Storage Oscilloscope and a pair of 1 MHz broadband transducers. A Negative going trigger pulse was used for excitation of the transducer. Water was used as a reference medium in the water bath here. The data obtained showed significant attenuation when the subject's heel was placed in vitro between the transducers. The values of *BUA* and *SoS* were noted. Data may have some errors due to calibration, motion artefacts and non-contact with sensors. To develop the analysis technique, Experimental data of in-vivo measurements of a trabecular bone sample provided by Dr. C.M. Langton was taken. A Fast Fourier Transform (FFT) window of length 512 and sampling frequency of 50 MHz was used in the algorithm. To calculate *BUA* and *SoS* the methods in section I-C were followed. But this time, we focused on the linear portion between 200 KHz to 600 KHz along with a digitization frequency of 100 MHz.

A Liquid Crystal Display (LCD) interface with Arduino Uno board to display values of Bone Mineral Density

(BMD) in gm/cm^3 was achieved. The values obtained in algorithm were serially transmitted at a baud rate of 9600 to display BMD. The formula [8, p. 89], to compute BMD is used here, arduino package was installed in the MATLAB workstation to establish a connection between arduino and Personal Computer (PC). The setup for the same is shown in “Fig. 5”.


III. OBSERVATIONS

The computed results of simulation for normal and osteoporotic subjects are shown in “table I”. Along with this data, results from in vivo measurements of the human feet are shown. As it can be seen, decrease in density leads to decrease in attenuation because of loss of bone due to disease. However, there was no significant change in speed of the subjects, although osteoporotic subjects showed a very minor increase. These values will be far from close to real data, because the parameters defined were used in nominal bone models and no porosity was considered for cancellous bone which plays a significant role in change in *BUA*. Nonetheless, the decrease in *BUA* values is of significance. It can be useful to study the role, effects of cancellous and cortical bone in measurement of *BUA* and *SoS*. Another interesting observation was the difference in values obtained from in-vitro and in-vivo measurements and the role soft tissue and other artefacts could play in these measurements.

IV. RESULTS

The *SoS* and *BUA* values were computed via simulation using the software SimSonic [9] with a 1 MHz Gaussian pulse and fractional bandwidth of 0.55 at 3 db and time duration of 3 μs .

Fig. 5. LCD and Hardware setup for display of results

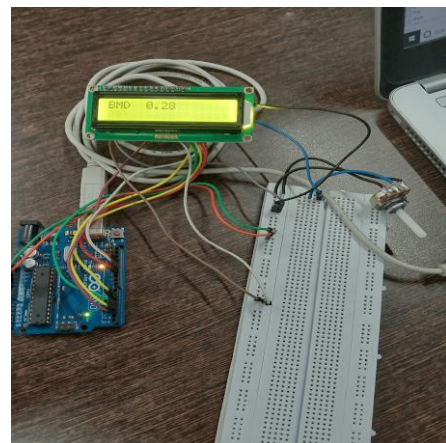

Measurement of Bone Density Parameters using Ultrasound and Hardware Development on bone Density Measurement

V. CONCLUSION

The *SOS* and *BUA* values using the techniques mentioned were calculated. Difference in *BUA* values were obtained for osteoporosis and normal samples in simulation. Moreover, variation in *BUA* values in the experimental setup with soft tissue and without soft tissue was noted. The 2D linear bone model served as a useful way of assessment of parameters during simulation in through mode. The *BUA* and *SoS* were close to the values reported in literature. Hence, ultrasound can be useful in estimation of bone density.

TABLE I
BUA AND *SoS* FOR NORMAL AND
OSTEOPOROTIC BONE IN DIFFERENT
SCENARIOS

Category	Bone Type	BUA in dB/MHz	SOS in m/s
Simulation	Trabecular (normal)	44.7	1504.064
Simulation	Trabecular(Osteoporosis)	35.2	1505.04
Experimental	Human Heel (in vitro)	29.69	1501.72

ACKNOWLEDGMENT

The work wouldn't have been possible without the guidance of Dr. Apurva Naik who gave me the wonderful opportunity to work in this project. A heartfelt gratitude to all my colleagues especially Mr. Kiran Kale, our teachers Prof. S.B. Somani, Prof. V.R. Tank and Cummins College of Engineering for Women, Pune for their support and involvement. A special thanks to Dr. C.M Langton for sharing his expertise and knowledge with us.

REFERENCES

1. Bossy, Emmanuel and Grimal, Quentin: Numerical Methods for Ultrasonic Bone Characterization. In: Bone Quantitative Ultrasound, Springer Netherlands, 181–228, 2011.
2. Haïat, Guillaume and Padilla, Frédéric and Peyrin, Françoise and Laugier, Pascal: Variation of Ultrasonic Parameters with Microstructure and Material Properties of Trabecular Bone: A 3D Model Simulation. In: Journal of Bone and Mineral Research, 665–674, 2007.
3. Biot, M. A.: Theory of Propagation of Elastic Waves in a Fluid-Saturated Porous Solid. I. Low-Frequency Range. In: The Journal of the Acoustical Society of America, 168–178, 1956.
4. Biot, M. A.: Theory of Propagation of Elastic Waves in a Fluid-Saturated Porous Solid. II. Higher Frequency Range. In: The Journal of the Acoustical Society of America, 179–191, 1956.
5. Aygün, Haydar and Attenborough, Keith and Postema, Michiel and Lauriks, Walter and Langton, Christian M.: Predictions of angle dependent tortuosity and elasticity effects on sound propagation in cancellous bone. In: The Journal of the Acoustical Society of America, 3286–3290, 2009.
6. P. Laugier and P. Droin and A.M. Laval-Jeantet and G. Berger: In vitro assessment of the relationship between acoustic properties and bone mass density of the calcaneus by comparison of ultrasound parametric imaging and quantitative computed tomography. In: Bone, 157–165, 1997.

7. T.HarnroongrojS, JiamamornratT and Tharmviboonsri: Characteristics of anterior inferior calcaneal cortex. In: Foot and Ankle Surgery, 1–4, 2017.
8. Barker R.: Non-Invasively Assessed Skeletal Bone Status and its Relationship to the Biomechanical Properties and Condition of Cancellous Bone. Cranfield University (2006).
9. Bossy et al, www.simsonic.fr, JASA 115, 2314–2324, 2004.

AUTHORS PROFILE



Kunal Khosla is an electronics and telecommunication graduate which he completed from Symbiosis Institute of Technology, Pune in the year 2015. He has a total work experience of two years in IBM as an application developer. He later decided to pursue his Masters of Technology in the field of VLSI and Embedded Systems, from MIT World Peace University, and currently is in the final year. He also secured first rank in the first year of his masters. His passions includes nature, dancing and hosting. He also holds a diploma in Business Management from Symbiosis Institute of Business Management. Email: khoslayr26@gmail.com



Dr. Apurva Naik graduated in Electronics Engineering from Shivaji University, Kolhapur in 1992. She has completed her M.E in Electronics from Shivaji University, Kolhapur in 2002. Dr. Apurva Naik has completed her Ph.D. in Electronics Engineering from RTM Nagpur university, Nagpur. She is working as Associate Professor in Electronics and Communication Engineering department of MIT since 2006. Earlier she worked with Padamshri Vittalrao Vikhe Patil College of Engineering Ahmednagar for 14 years. She has one year industrial experience in quality control department of Microcontrols, Pune. She has 25 years of teaching experience in the field of Electronic devices and Circuits, Image processing and computer vision, electronics design, Electronic Product Design, Embedded Processor, Embedded System Design, Computer Organization and Architecture and Miniprojects. She has been paper setter for many subjects of SPPU like Computer Organization and Architecture, Electronic Devices and Circuits, Electronic Product design. Participated in syllabus design for Electronic Product Design and Embedded System Design. Under her guidance 12 ME projects have been completed. Dr. Naik has authored 3 research papers for the International Conferences held in the world like Venice, Paris, Cyprus in 2013, 2014 and 2016 respectively. She has published 9 more papers in international conferences and journals. Two of her international publications received best paper award in the conference and journal extension. Dr. Naik also has two patents published. Email: apurva.naik@mitpune.edu.in