

Knee-Jerk Cardiopulmonary Resuscitation (CPR) Machine

Ms. E. Niranjana, S. Saranya, S. Kaarika Sree, B. Keerthana, J. Gajalakshmi

Abstract: *Cardiopulmonary resuscitation method is used to save more number of peoples from the neurological problem. In this case, the neurological problem denotes brain death. This brain death is mainly caused due to cardiac arrest and happen within 4 to 5 minutes. To avoid this problem we go for cardiopulmonary resuscitation method. It will be helpful to relieve the patient from cardiac arrest. The manual CPR is not that much efficient when compared to automatic CPR because, the experts who are giving CPR to the patient are cannot able to give the continuous CPR to the patient but, the automatic CPR machine is able to give the continuous CPR to the patient. The article reviews such kind of automatic devices. The automatic CPR machine already exists. But, the cost of that machine is high. So we intended to design the low cost CPR machine. This is achieved by replacing the component like Arduino microcontroller and solenoid lock. The replaced component also do the same work like in the high cost CPR machine.*

Keywords : *CPR (Cardiopulmonary Resuscitation), Arduino Microcontroller, solenoid lock, knee-jerk devices.*

I. INTRODUCTION

In cardiac arrest, the heart abruptly stops beating without prompt intervention, it can result in the person's death. The main symptom is loss of consciousness and unresponsiveness. This medical emergency needs immediate CPR or use of a defibrillator. Hospital care includes drugs, an implantable device or other procedures. If not treated immediately, sudden cardiac arrest can lead to death. With fast appropriate medical care like CPR will be provided, then the survival of the patient is possible. Giving CPR can improve the chance of survival until emergency workers arrive. Cardiac arrest is one of the leading causes of death worldwide and it is also lead to coma due to acute embolism. But, this embolism managed by cardiopulmonary resuscitation(CPR) and extracorporeal membrane oxygenation with an excellent neurological recovery. The use of CPR in such cases is believed to reduce the mortality rate and increase the survival rate with good neurological outcomes. It saves nearly 4,00,000 to 5,00,000 peoples in every year and we believe this will be increased in the upcoming year.

Revised Manuscript Received on October 05, 2019.

Ms. E. Niranjana, Assistant Professor in Department of Biomedical Engineering Rajiv Gandhi College of Engineering and Technology, Puducherry.

Ms. S. Saranya, pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry

Ms. S. Kaarikaasree, pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry

Ms. B. Keerthana, pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry

Ms. J.Gajalakshmi, pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry

The effectiveness of the CPR depends on the quality of the resuscitation procedure. The parameters of the CPR machine are chest compression rate, chest compression force and execution timing. The chest compression rate is 30 compression per minute and 2 rescue breath and the chest compression force ranges from 100 to 125 pounds of force. The execution time for CPR is about two minutes before calling for help. Continue CPR until you see signs of life or until medical personnel arrive. These parameters are stated in the basis of AHA guidelines. The distance between the patient chest and the piston varies by patient to patient based on their physical appearance. Mostly the distance between chest and piston are 1.5inches to 2inches. During the time of first aid, automatic CPR machine is very helpful to lift the patient from one place to another place. The rigid stretcher is used during the transportation of the patient from the scene to the ambulance, the compression can continue uninterrupted all the time. The devices aimed at replacing completely the manual CPR.


II. OBJECTIVE

The objective of project is to reduce the cost of the CPR machine. It is achieved by the replacement of the component in the existing CPR machine. The replaced component also do the same work as the component in the existing CPR. But, it is cost effective. The existing CPR machine price nearly 1,00,000 and our project reduce the price to 50,000. So, the ultimate aim our paper is achieved.

III. EXISTING SYSTEM


In the existing system, direct current is used as a power supply. The electronic unit gives supply to the motor and the timer circuit. The mechanical elements like gear assembly controls the speed of the DC motor. The DC motor is connected with the rod shape projection and disc shape projection. These two projection combine to give compression to the patient. Here the compression rate is controlled by the timer circuit. IC 555 is used in the timer circuit. The overall components used in the existing technique are DC motor, battery or DC supply, IC 555, gear assembly, disc.

Knee-Jerk Cardiopulmonary Resuscitation (CPR) Machine

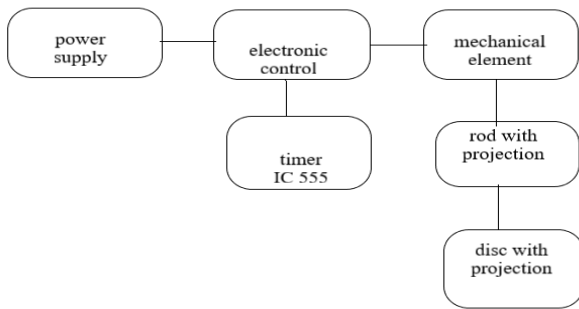

IV. PROPOSED SYSTEM

In the proposed system battery or DC power supply is used as a power supply as same in the existing system. The Arduino board is used to control the compression rate, which is act as a timer circuit in the existing system. The world health organization was already mentioned the word “In the future, microcontroller replace the timer circuit”. The time delay program is fed into the Arduino board to perform the timer function. The combined structure of projection in the existing technique was replaced here as a piston . piston is used to give the compression to the patient. There is no need of motor here to control the piston movement. Relay module is used for the delay purposes.

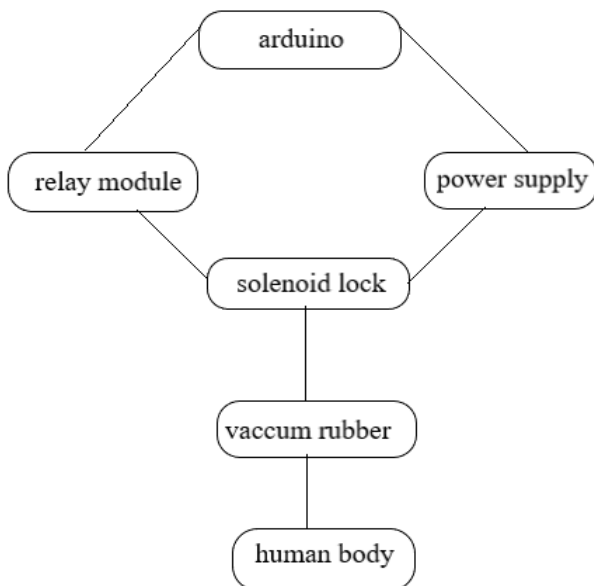

V. DESCRIPTION OF SCHEME


The components we are using here to reduce the cost of the CPR machine are Arduino microcontroller, relay module, power supply, piston, vacuum rubber pad. In our project, the Arduino board replace the function of the timer and piston replaces the function of rod & disc shape projection in the existing system. The main components in our project are,

- Arduino microcontroller
- Piston
- Relay module

The description of the above mentioned components are given below,


Arduino Microcontroller

Arduino microcontroller contain 14 digital pins and 6 Analog pins. In this paper, the 14 digital pins are used to give input or output for our project using pinMode(), digitalWrite() and digitalRead() functions. DC current for 3.3V out is 50mA and the DC current for 3.3V in is 1A. It is supplied with the external adapter. The recommended supply voltage ranges from 16 to 20V and the clock speed is 16MHZ. we fed the coding into the Arduino board to perform the timer function. A maximum of 40mA is the value that must not be exceeded on any input and output pin to avoid permanent damage to the microcontroller. The memory used in Arduino is EPROM, so we can able to upload the more number of program.

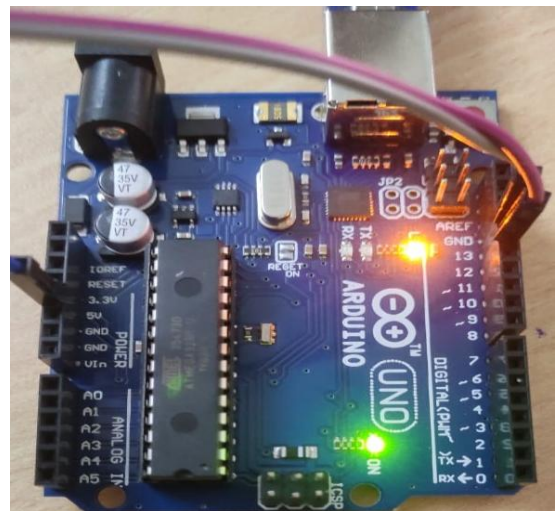

Piston

Piston is the disc shape metal connected with the rod shaped projection. These structure is used to give the compression to the patient. The speed of the piston is controlled by the relay module. If the speed of the piston increases, the relay module break the loop and save the patient from danger.

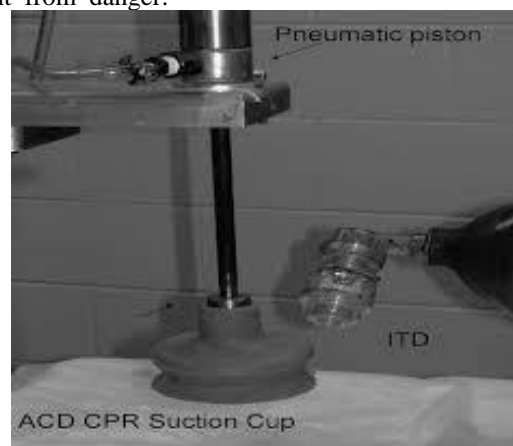

Relay Module

The relay is an electrically operated switch that can be turned on or off, letting the current go through or not, and can be controlled with low voltages, like the 5v provided by the Arduino pins. Relay module using here is single phase or single channel relay module. This module is powered with 5V, which is appropriate to use with an Arduino.



Manual and Automatic CPR Devices

The CPR device is categorized into two types, they are manual and automatic devices. Fig 2 shows the one example for manual CPR machine (a) CPR PRO cradle and then the three automatic devices are (a) EM-CPR, (b) life stat, and (c) LUCAS. The above mentioned these automatic components are shown given below.



Fig.1 Function of CPR



Fig.2 Manual CPR Machine

The manual devices are auxiliary component to perform the step-by-step procedure to give proper massage to the rescuers. In some devices, it is used to reduce the fatigue of the rescuers for the more efficient compression process.



Fig.3 Automatic CPR Machine

The automatic CPR machine are able to provide the automatic chest compression to the patient with proper rate and depth. So the automatic CPR machine is more helpful than the manual CPR machine. The different types of automatic CPR machine are available. These CPR machine are classified based on the their structure and compactness.

VI. CONCLUSION

This paper review the advantages of automatic CPR machine and how it will be implemented in the affordable price. This is achieved by the replacement of the solenoid lock. We will see the output in the form of piston movement by using manikins. This manikins are very helpful to find out the compression rate & force.

REFERENCES

1. Neumar RW, Otto CW, Link MS et al. Part 8, "Adult advanced cardiovascular life support: 2010 American heart association guidelines for cardiopulmonary resuscitation and emergency cardiovascular care", *Circulation* 2010; 122: S729-167.
2. Yu T, Weil MH, Tang W, et al. "Adverse outcomes of interrupted precordial compression during defibrillation" *Circulation* 2002; 106: 368-372.
3. Hightower D, Thomas SH, Stone CK, et al. "Decay in quality of closed-chest compressions over time" *Ann Emerg Med* 1995; 26: 300-303.
4. Ochoa FJ, Ramalle-Gomara E, Lisa V, et al. "The effect of rescuer fatigue on the quality of chest compressions" *Resuscitation* 1998; 37: 149-152.
5. Leary M and Abella BS. "The challenge of CPR quality: improvement in the real world" *Resuscitation* 2008; 77: 1-3.
6. Aliverti A, Bovio D, Fullin I, et al. "The abdominal circulatory pump device" US20120016280-A1 patent, 2012.
7. Jung E, Lenhart S, protopopescu V, et al. "Optimal control applied to a thoraco-abdominal CPR model", *Math Med Biol* 2008; 157-170.
8. Halperin H, Berger R, Chandra N, et al. "Cardiopulmonary resuscitation with a hydraulic-pneumatic band", *Critcare Med* 2000; 28: N203-N206.
9. Brooks SC, Hassan N, Bigham BL, et al. "Mechanical versus manual chest compressions for cardiac arrest", *Cochrane Database Syst Rev* 2014; 2: CD007260.
10. Guyette FX, Reynolds JC and Frisch A. "Cardiac arrest resuscitation", *Emerg Med Clin North Am* 2015; 33: 669-690.
11. Jones AY. "Can cardiopulmonary resuscitation injure the back? Resuscitation", 2004; 61: 63-67.
12. Omori K, Sato S, Sumi Y, et al. "The analysis of efficacy for AutoPulse system in flying helicopter", *Resuscitation* 2013; 84: 1045-1050.
13. Ventzke MM, Gassler H, Lampl L, et al. "Cardio pump reloaded: in-hospital resuscitation during transport", *Intern Emerg Med* 2013; 8: 621-626.

Knee-Jerk Cardiopulmonary Resuscitation (CPR) Machine

14. Halperin H and Carver DJ. "Mechanical CPR devices", *Signa Vitae* 2-10; 5: 69-73.
15. Fribreg H and Rundgren M. Submersion, accidental hypothermia and cardiac arrest, "Mechanical chest compressions as a bridge to final treatment: a case report", *Scand J Trauma Resusc Emerg Med* 2009; 17: 7.

AUTHORS PROFILE



Author 1 - Ms. E. Niranjana received BE Degree in the stream of Electronics and communication engineering from the IFET college of Engineering & Technology in 2014, ME in Applied Electronics from CK College of Engineering & Technology in 2016. Her primary duty is teaching profession and having 3 years of experience. She is currently working as an Assistant Professor in Department of Biomedical Engineering Rajiv Gandhi College of Engineering and Technology, Puducherry. She published 5 papers in international and national journal and attended conferences. Her interests include Integrated circuits and circuit theory.



Author 2 - Ms. S. Saranya pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry in the year 2020.



Author 3 - Ms. S. Kaarikaasree pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry in the year 2020.



Author 4 - Ms. B. Keerthana pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry in the year 2020.



Author 4 - Ms. J. Gajalakshmi pursuing her B.Tech, biomedical engineering in Rajiv Gandhi college of engineering and technology, Puducherry in the year 2020.